
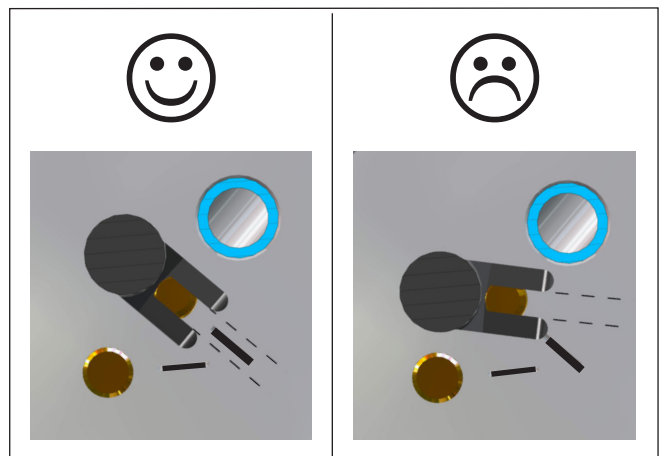
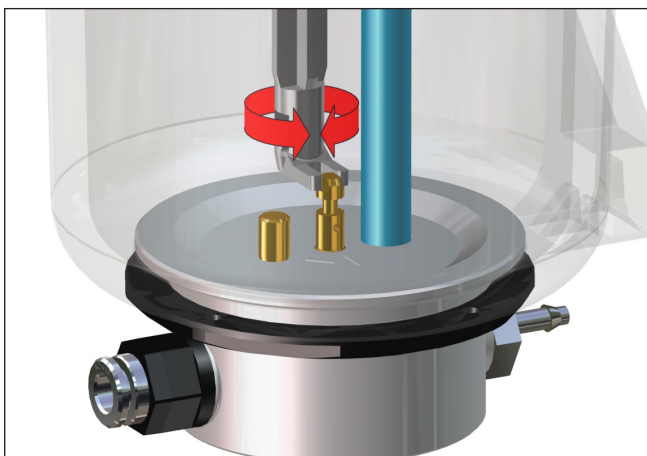
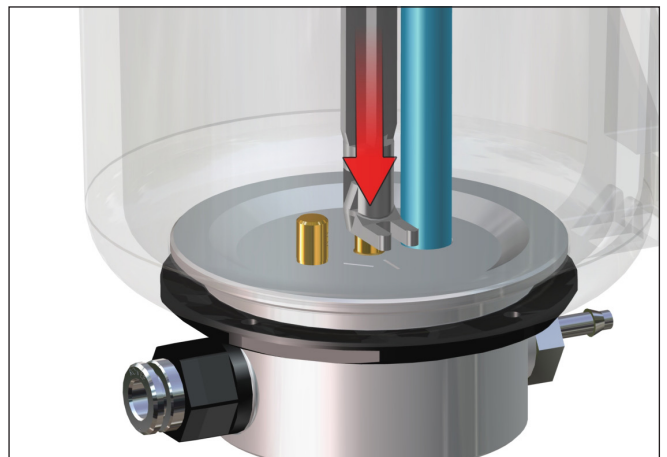
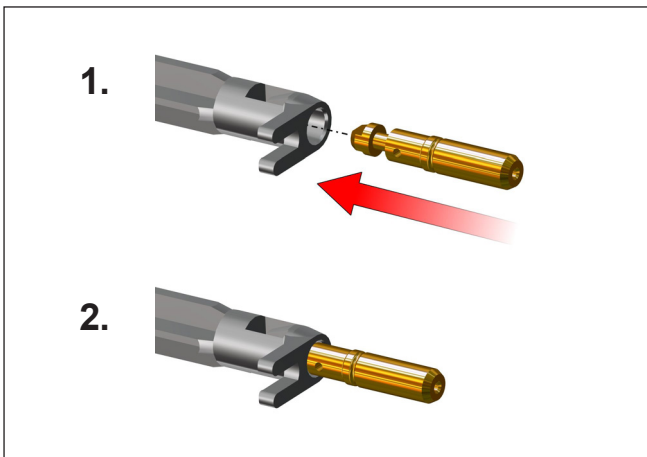
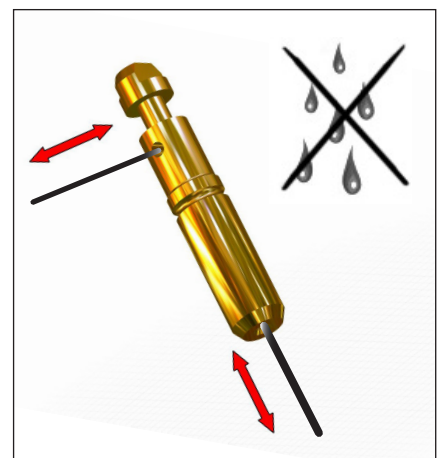
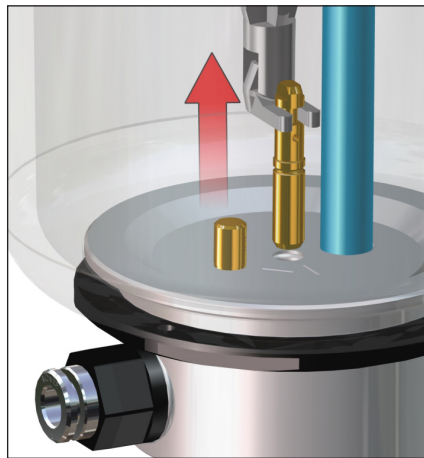


25 - 70 µm (500 - 200 mesh)

Dosierdüse reinigen • Cleaning the dosing nozzle • Nettoyage de la buse de dosage • Pulire l'ugello dosatore • Limpiar la boquilla dosificadora • Чистка дозирующего сопла • 定量噴咀・流入ノズルのクリーニング・ 분사노즐 청소하기

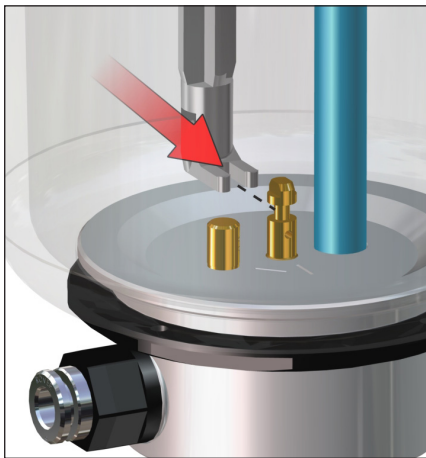

70 - 250 µm (200 - 60 mesh)

Dosierdüse reinigen • Cleaning the dosing nozzle • Nettoyage de la buse de dosage • Pulire l'ugello dosatore • Limpiar la boquilla dosificadora • Чистка дозирующего сопла • 定量噴咀・流入ノズルのクリーニング・ 분사노즐 청소하기

